



SUPERVISOR OF SHIPBUILDING, CONVERSION AND REPAIR, USN
TWELFTH NAVAL DISTRICT
SAN FRANCISCO, CALIFORNIA 94135

IN REPLY REFER TO:
 1700-54
 9900

12 DEC 1974

From: Director, NAVSEA Industrial Support Office, San Francisco, California 94135
To: Commander, Naval Electronic Systems Command (CODE 48053)
 Naval Electronic Systems Command Headquarters, Washington, D. C. 20360

Subj: AEC Byproduct Material License No. 04-13597-02

Ref: (a) NAVELEX ltr 4805:GNM:mar 9900 Ser 397-48053 of Jun 25, 1974

- Encl:**
- (1) Completed form AEC-314 (2 copies)
 - (2) NAVELEXSYSENGCEN, Vallejo memo: Radioactive Survey; results of, dtd 6 Dec 1974 (2 copies)
 - (3) Set of 5 Sketches of areas surveyed (2 sets)
 - (4) Copy of AEC Byproduct License No. 04-13597-02 w/amendment No. 01 (2 copies)

1. Reference (a) requested additional data known to be required for license termination. Enclosures (1) through (4) provide the requested data. Enclosure (1) is the Certificate of Disposition of Materials. Enclosure (2) is a report of a survey for radioactivity in areas where radioactive materials were used or stored. Enclosure (3) is a set of sketches of the surveyed areas showing grid location and identification of wipe tests. Enclosure (4) is a copy of the Hunters Point Naval Shipyard Byproduct Material License to be terminated.

2. The survey was made by the Shipyard Radiac Coordinator and NAVELEXSYSENGCENVALLEJO who provided the required instrumentation and qualified personnel. The Radiac Coordinator, Mr. L. Kearney will no longer be available after the end of the year. Person to contact in this and other similar matters is Mr. F. Stivender, Code 1700, Head, Maintenance and Security Department, NAVAL SEA Industrial Office, San Francisco, CA. 94135, Phone: COM (415) 641-2618, AV. 799-2618. Mr. Stivender is the last on-site person with continuity of knowledge of the shipyards operations with radioactive materials and instruments. The residual files concerning these matters will be in his custody.

3. Termination of the Byproduct Material License should be sent to: Director, NAVSEA Industrial Support Office (CODE 1700), San Francisco, CA. 94135.

P. D. Kjeldgaard

P. D. KJELDGAARD

4805

Copy to:
 NAVELEXSYSENGCEN VALLEJO (Attn: R. J. Reid, Code 034)

1217 037 074

DEPARTMENT OF THE NAVY

Memorandum

DATE: 6 Dec 1974

FROM : L. P. McNeice, Code 034

TO : L. Kerney, Code 630.3, San Francisco, CA 94135

SUBJ : Radioactive Survey; results of

1. As requested, the following report is submitted on wipe tests performed at the locations indicated. In addition, surveys made with both an AN/PDR-56 and an E-140N at the same locations, indicated no detectable activity.

- | | |
|-----------------------------|--------|
| (a) Building 113A | N.D.A. |
| (b) Building 146 | N.D.A. |
| (c) Building 214, RM 105 | N.D.A. |
| (d) Building 253, 6th Floor | N.D.A. |
| (e) Building 351A | N.D.A. |


L. P. McNEICE

ENCLOSURE (2)

AE-314
(1-74)

UNITED STATES ATOMIC ENERGY COMMISSION

CERTIFICATE OF DISPOSITION OF MATERIALS
(ALL BLOCKS MUST BE COMPLETED)

LICENSEE NAME AND ADDRESS:

Department of the Navy
Hunters Point Naval Shipyard
San Francisco, California 94135

LICENSE NUMBER:

04-13597-02

LICENSE EXPIRATION DATE:

March 31, 1975

The licensee and any individual executing this certificate on behalf of the licensee certify that (check appropriate item(s) below)

- A. No materials have been procured by licensee.
- B. All materials procured and/or possessed by licensee under license number shown above, have been:

Transferred to: Naval Ordnance Laboratory, White Oak,
Silver Spring, Maryland 20910

which has license number: 19-00166-10

C. Disposed of in compliance with 10 CFR 20.

D. Licensed under license number _____ issued by:

_____, an Agreement State pursuant to Section 274 of the Atomic Energy Act of 1954, as amended.

REMARKS: (if additional space is needed, use reverse side)

L. G. Kearney
L. G. Kearney, Radiac Coordinator
Signature of Certifying Official
3/12/74
Date

Please return to:
U.S. Atomic Energy Commission
Office of Regulation
Directorate of Licensing
Washington D.C. 20545


ENCLOSURE (11)

Bldg 13A

8/15/79

Radiographers Vault & Waste Disposal Storage

Note: Used for Waste Disposal Storage from approx 10/73 to 6/74

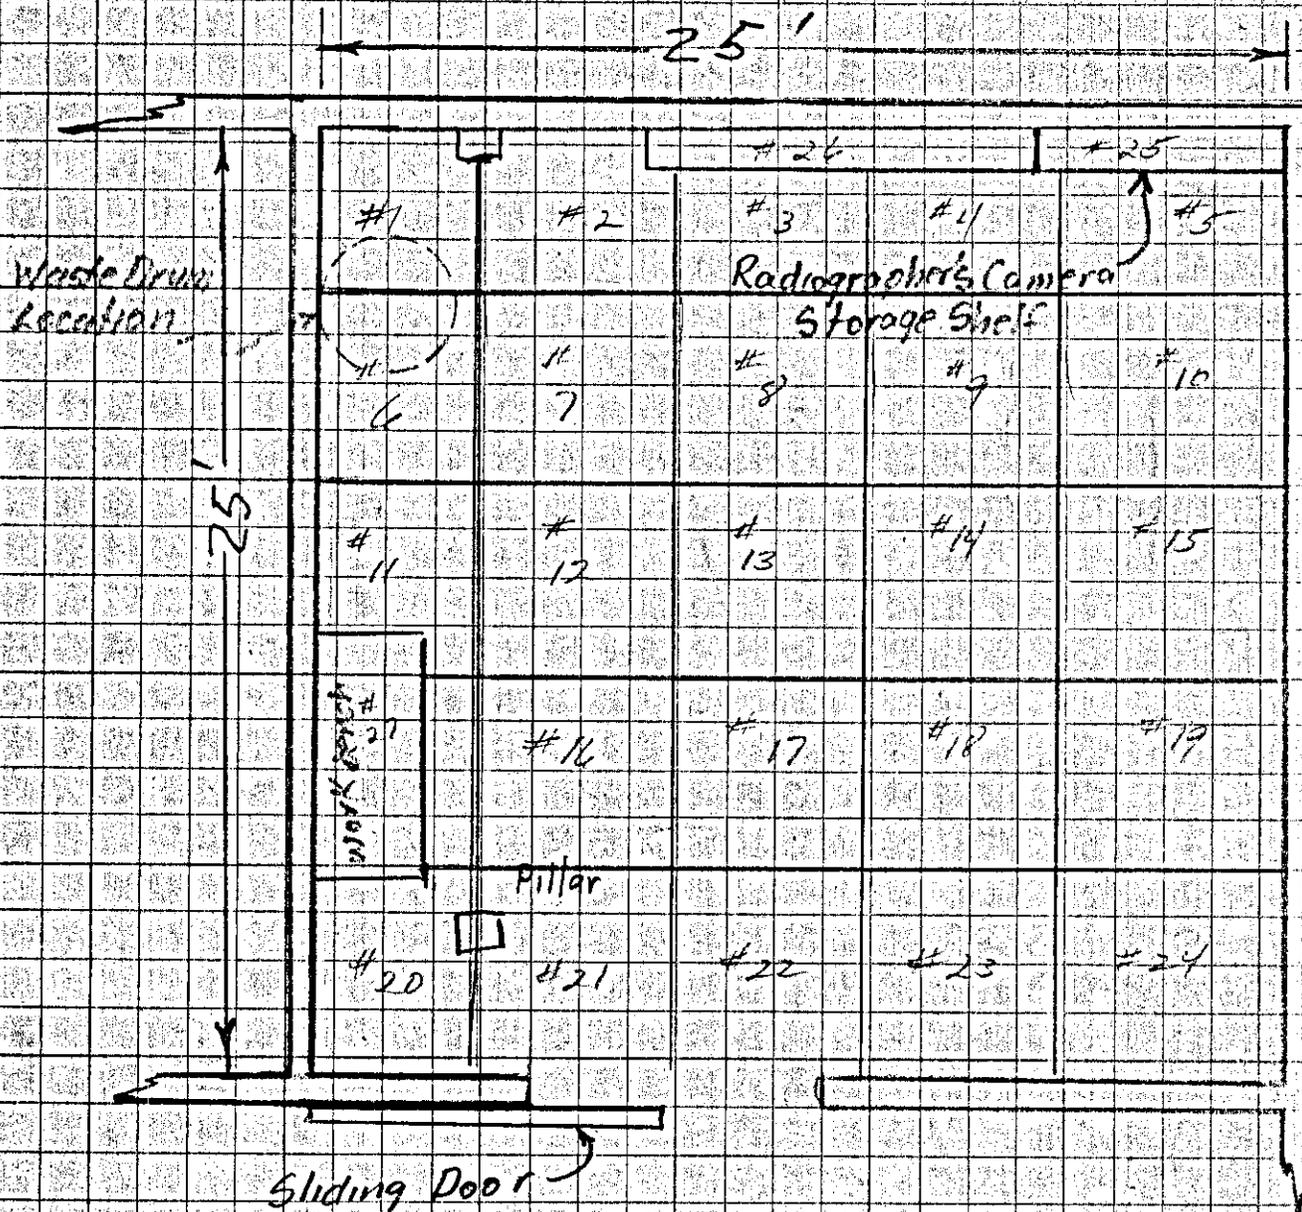

Scale 1" = 1 foot

Construction: Concrete

29 WIPES
 2 WIPE ON SOURCE TRANSPORT
 BOX
 (Walls & Floor)


Bldg 146 (Ground floor)

8/21/74

Radioactive Waste Disposal Drum Storage

Note: Used for Waste Disposal Storage until approx 10/53

Drum Location

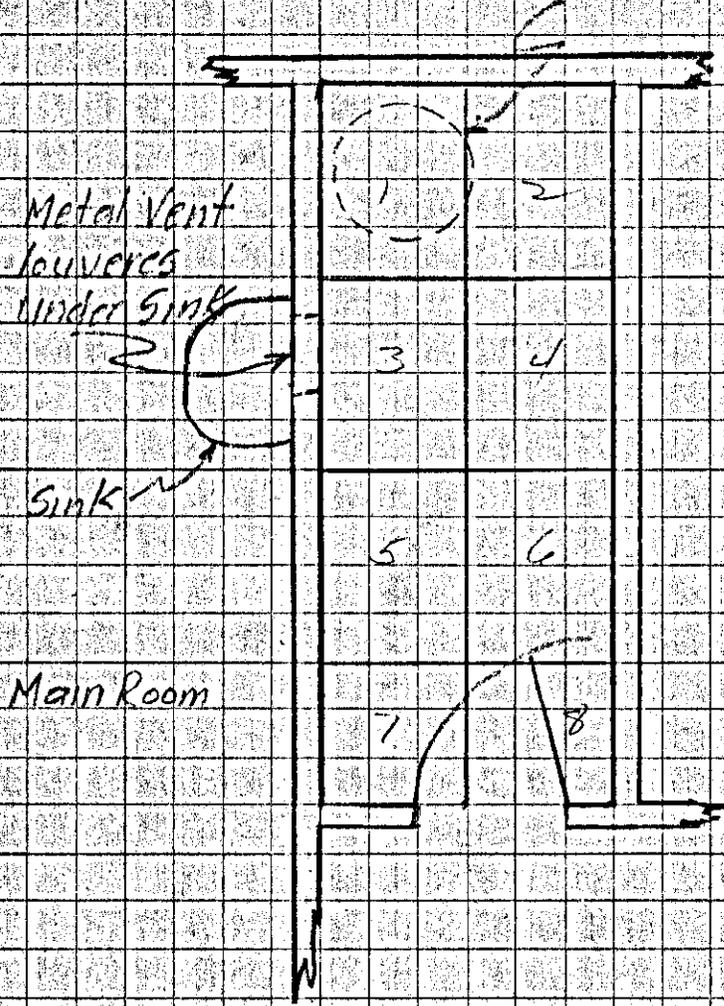


Scale 1 square = 1 ft.

Construction: concrete walls & floor

Bldg 214 Rm 105


8/15/74

Health Physics Counting Rm.

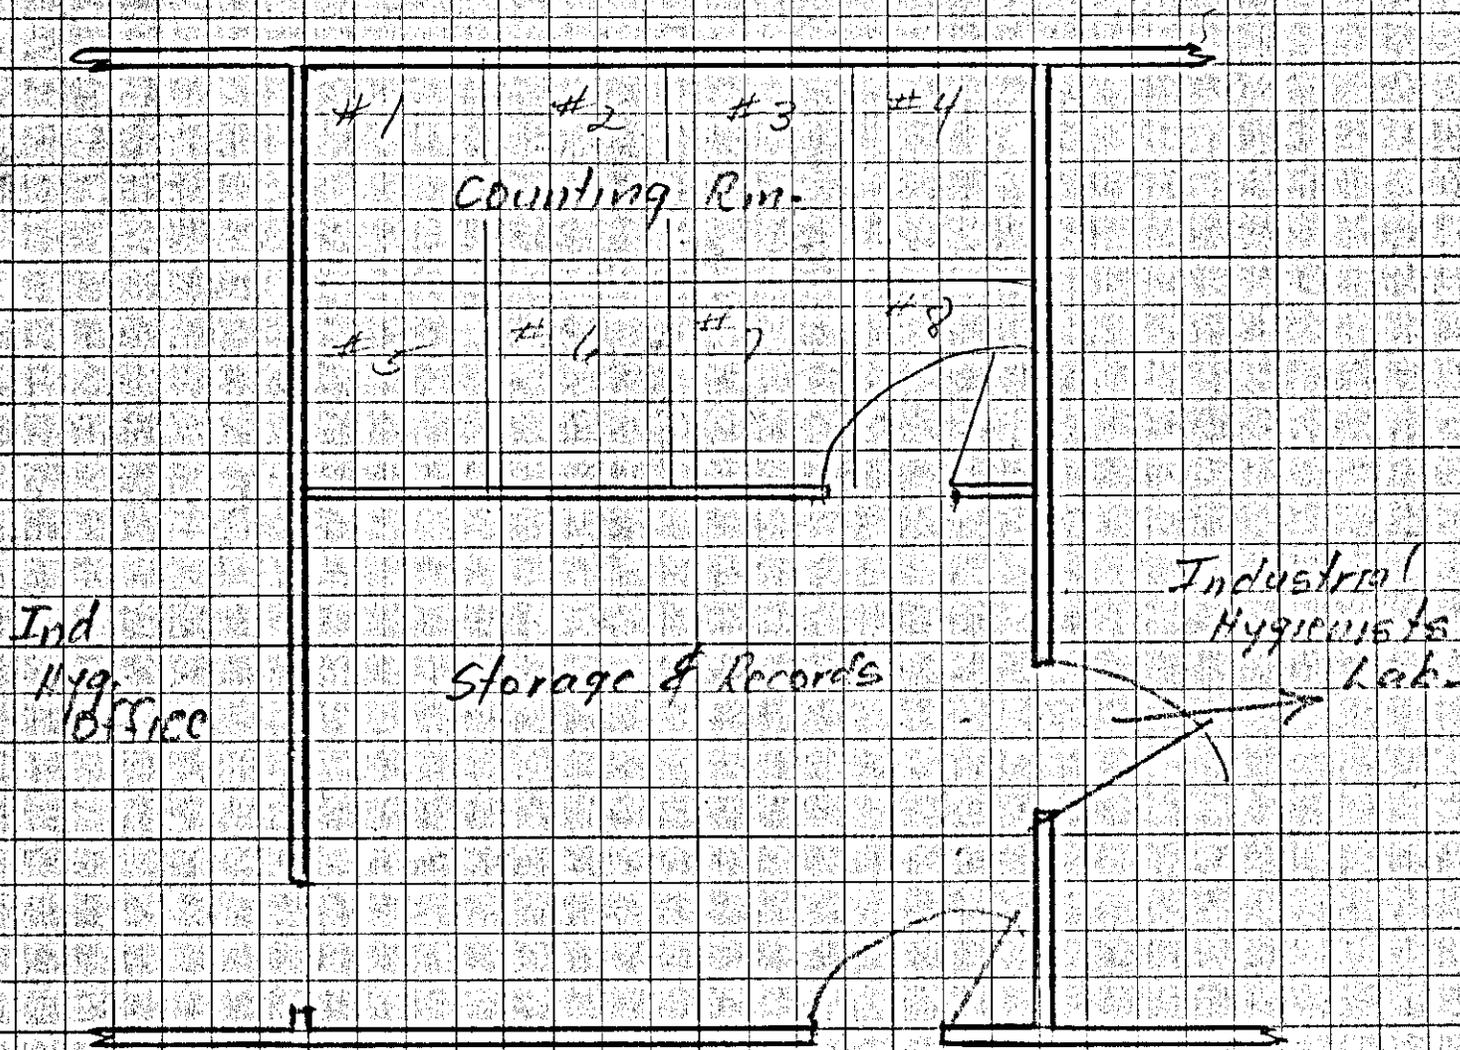

Scale 1 Square = 1 foot

Construction: Wood frame

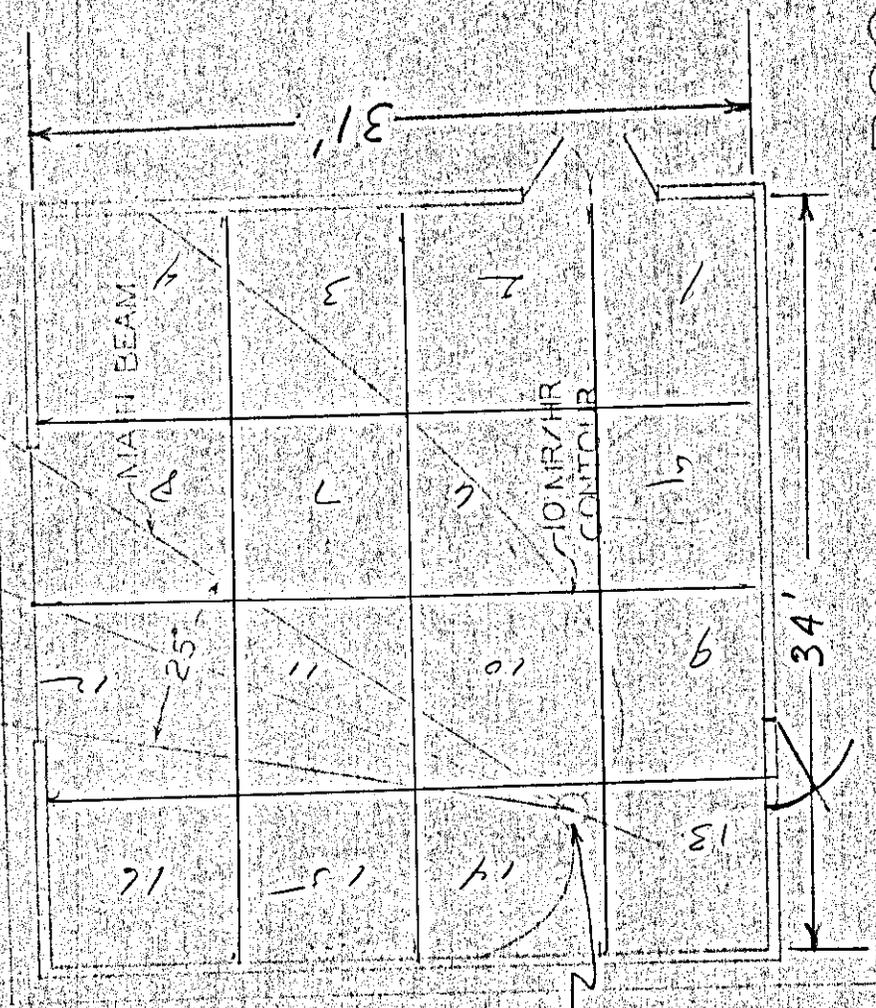

Construction: Concrete
Walls & Floor
Measurements made 8/21/79


CALIBRATION ROOM
BLDG 253 6TH FLOOR

SFNS SKETCH NO. 10555
CODE 288 3/20/56

Bldg 35 A

8/15/74

Radiac Repair Facility

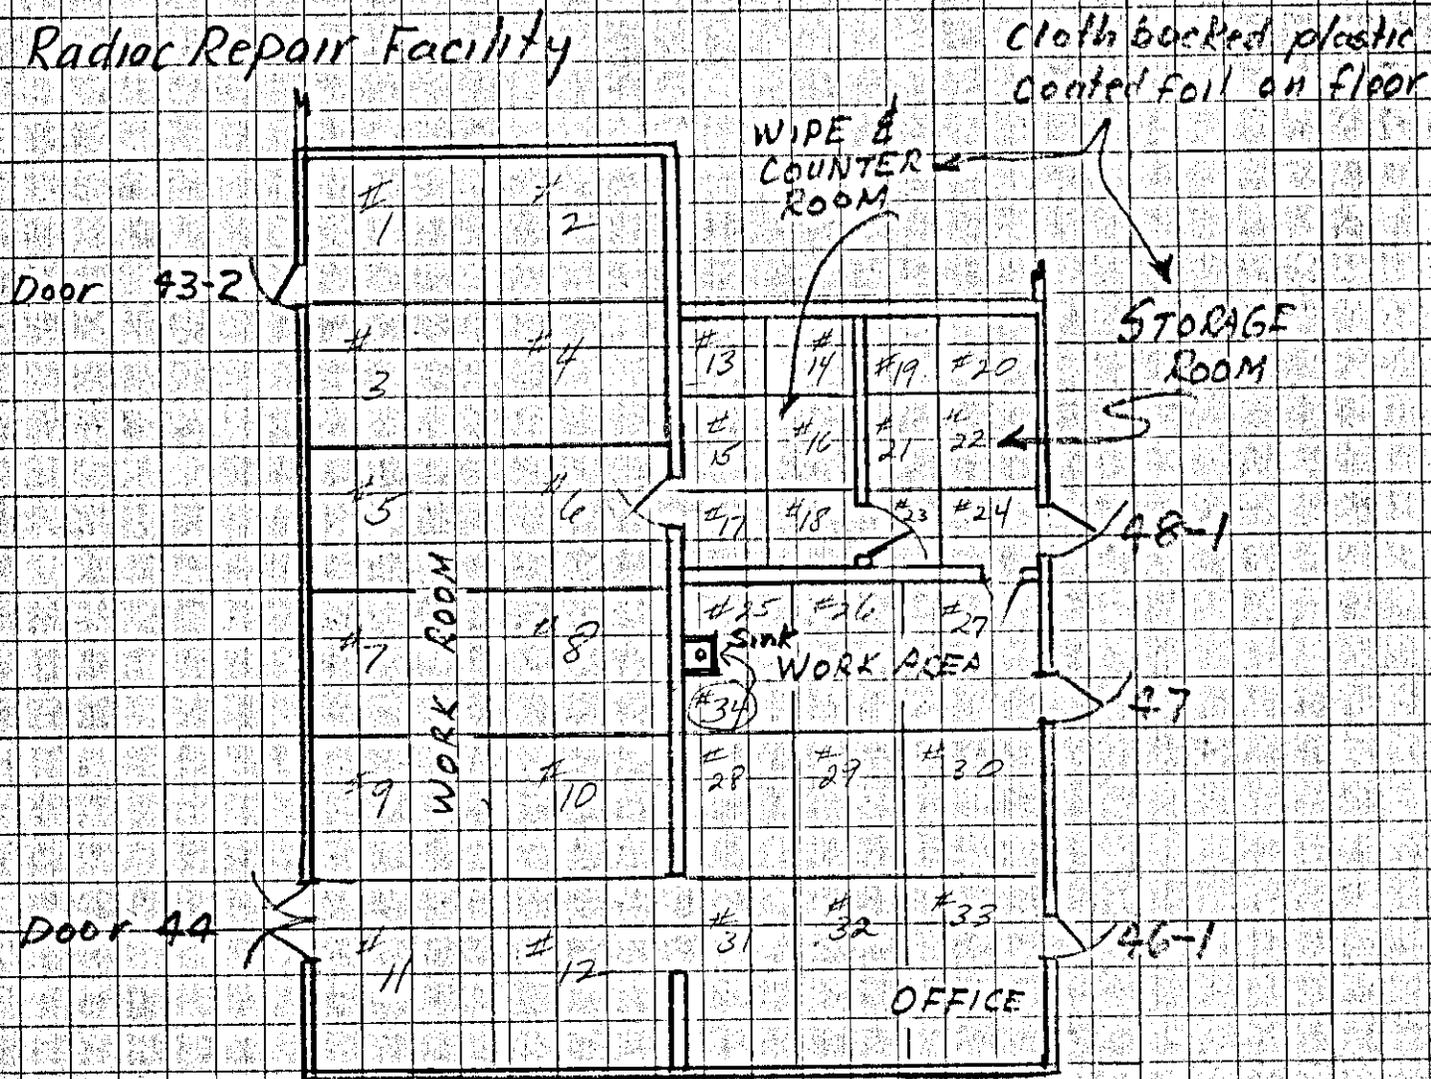

Scale: 1 Square = 3 ft

Construction: Wood frame